

Figure 1 (Prior Art)

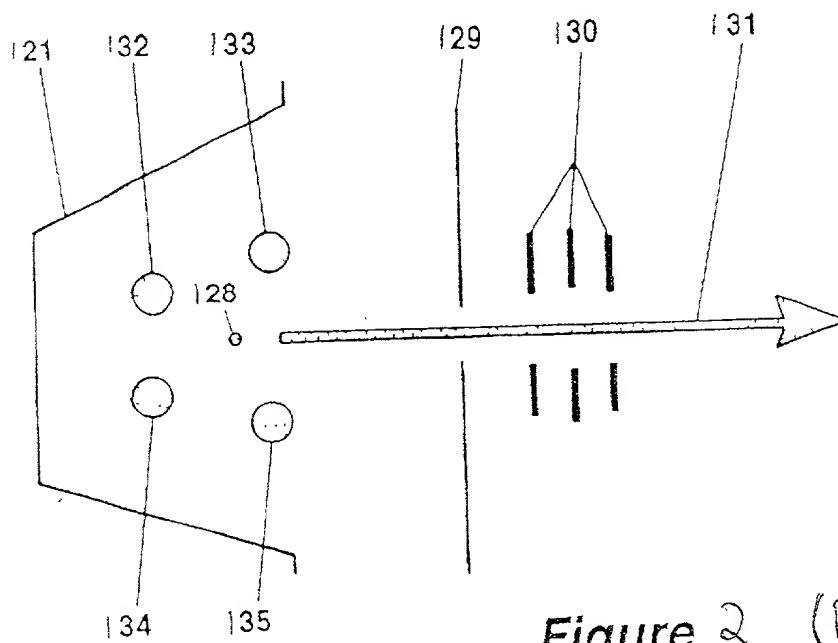


Figure 2 (Prior Art)

32 ↓

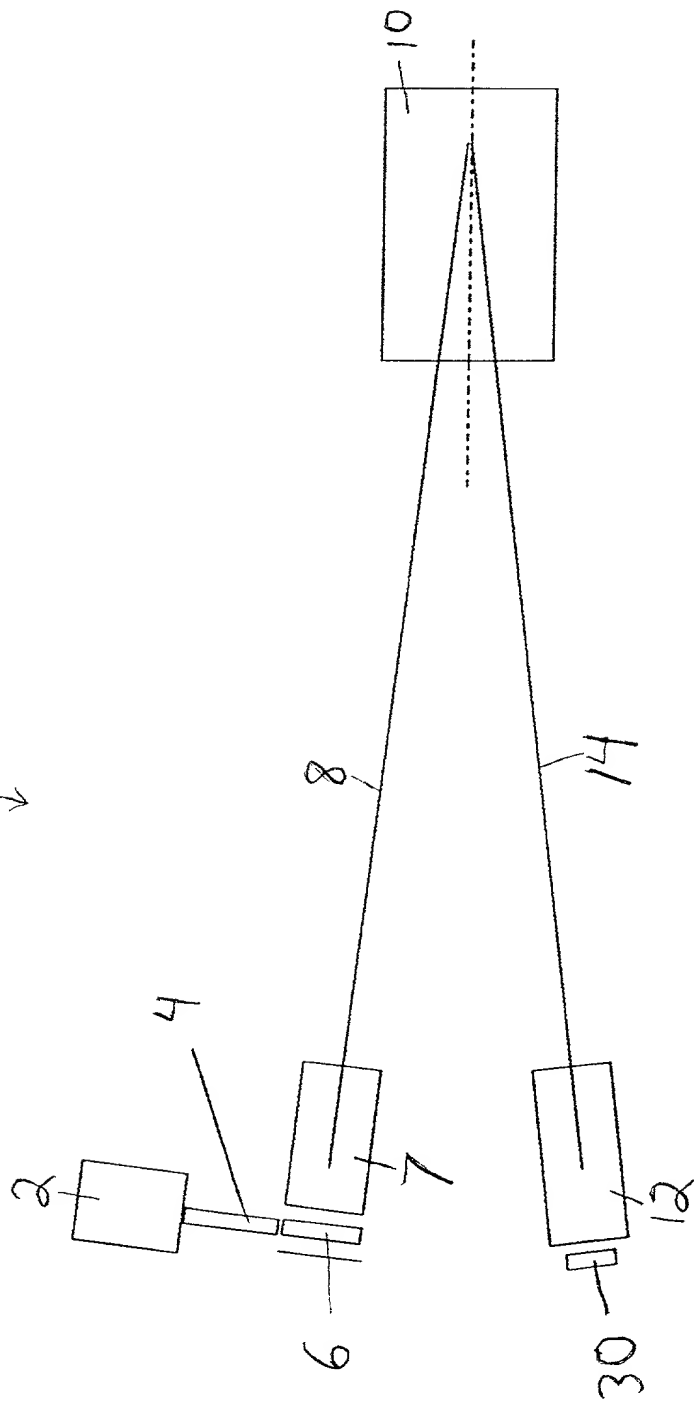


Figure 3

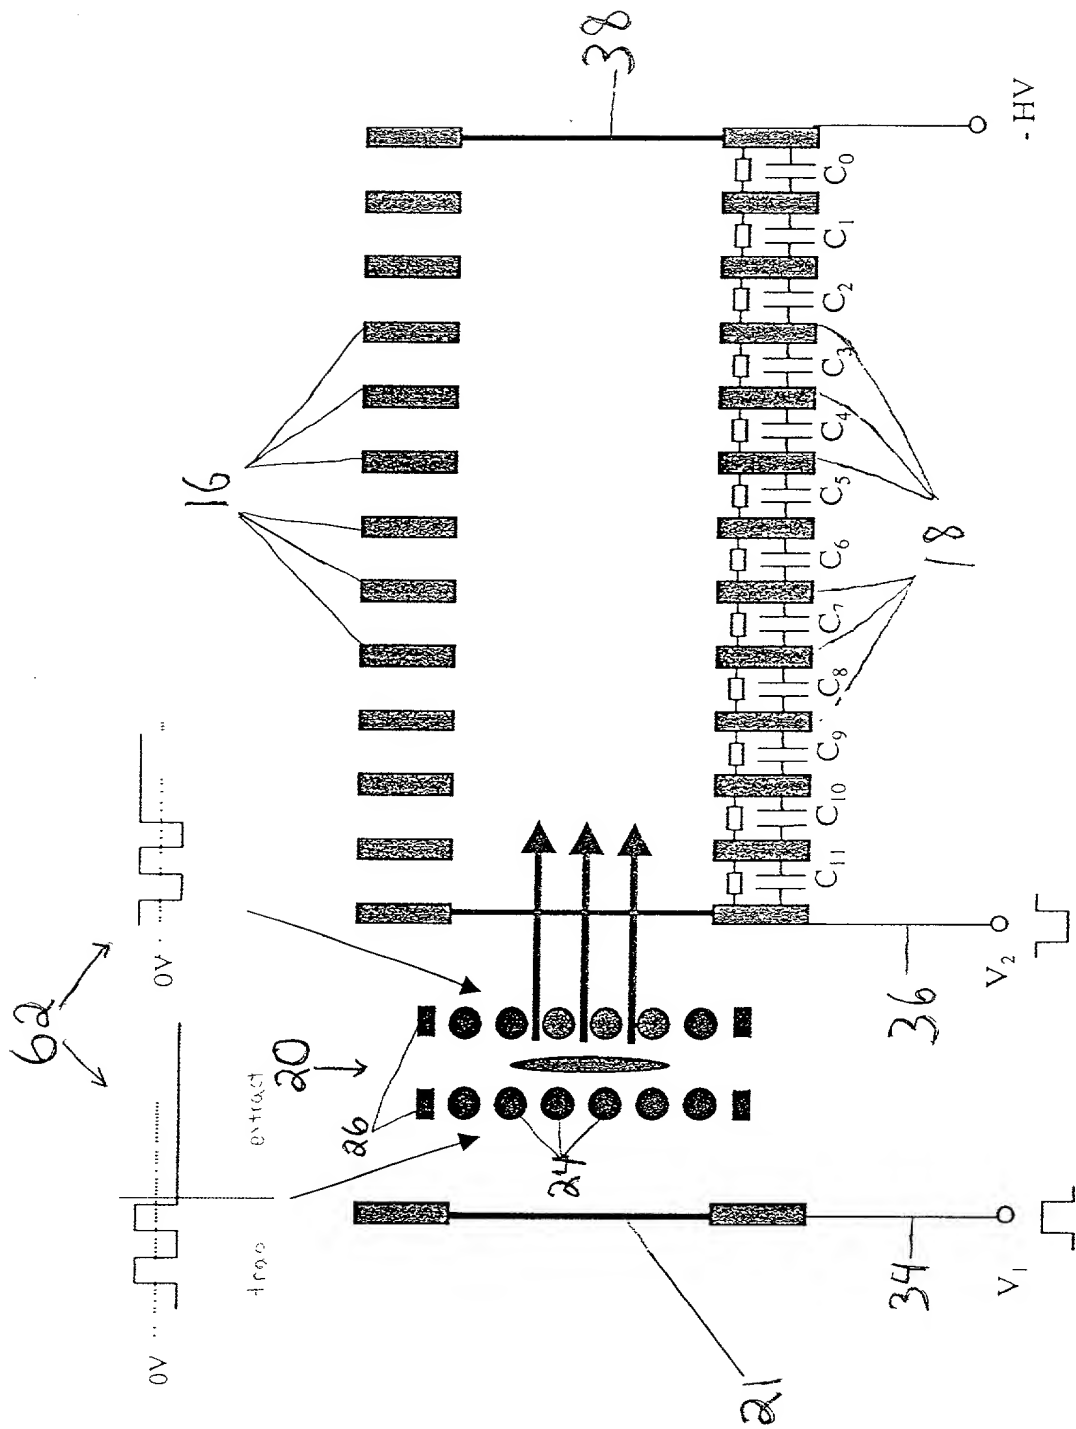


Figure 4

20

24


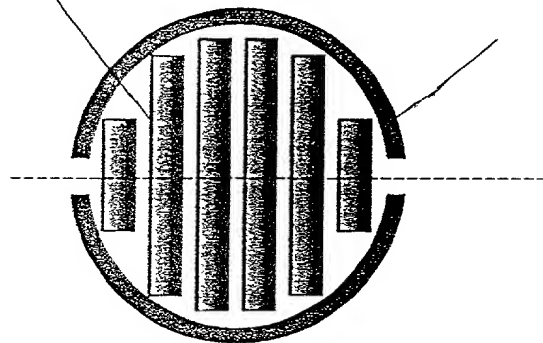



Figure 5A

28

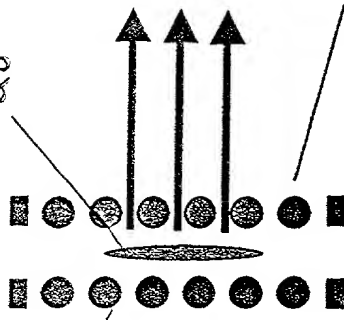

0V

63



26

trap

extract

52

Figure 5B

22 ↓

26
20 ↓

42

40

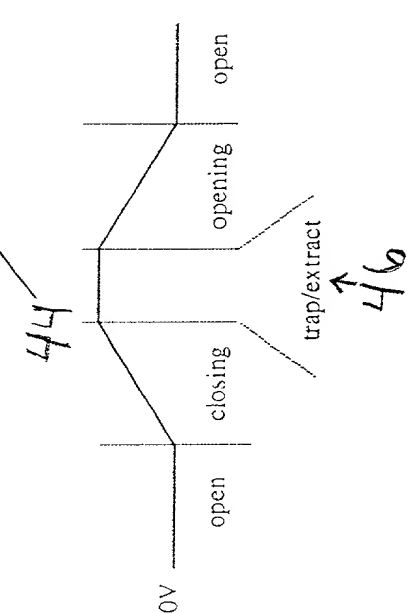
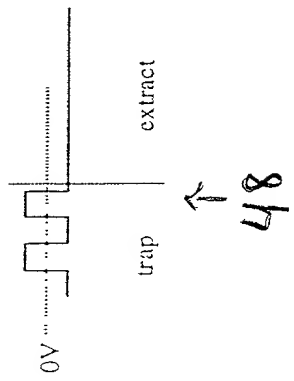


Figure 6

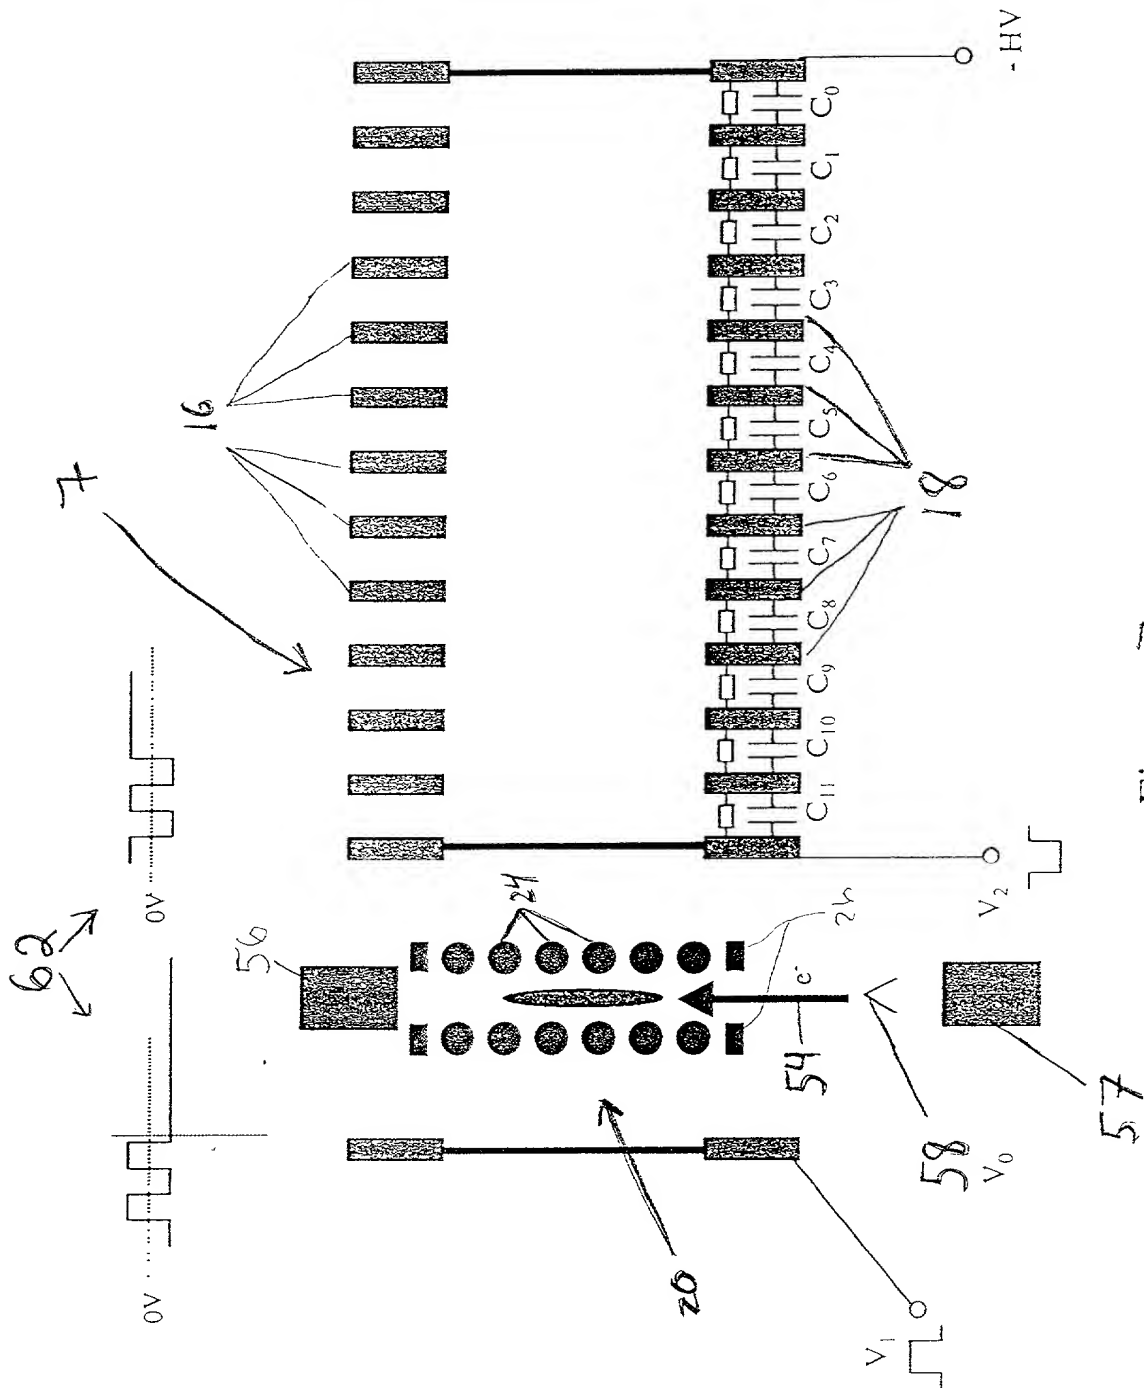


Figure 7

TOP-TECH

angio li gate open 300 us

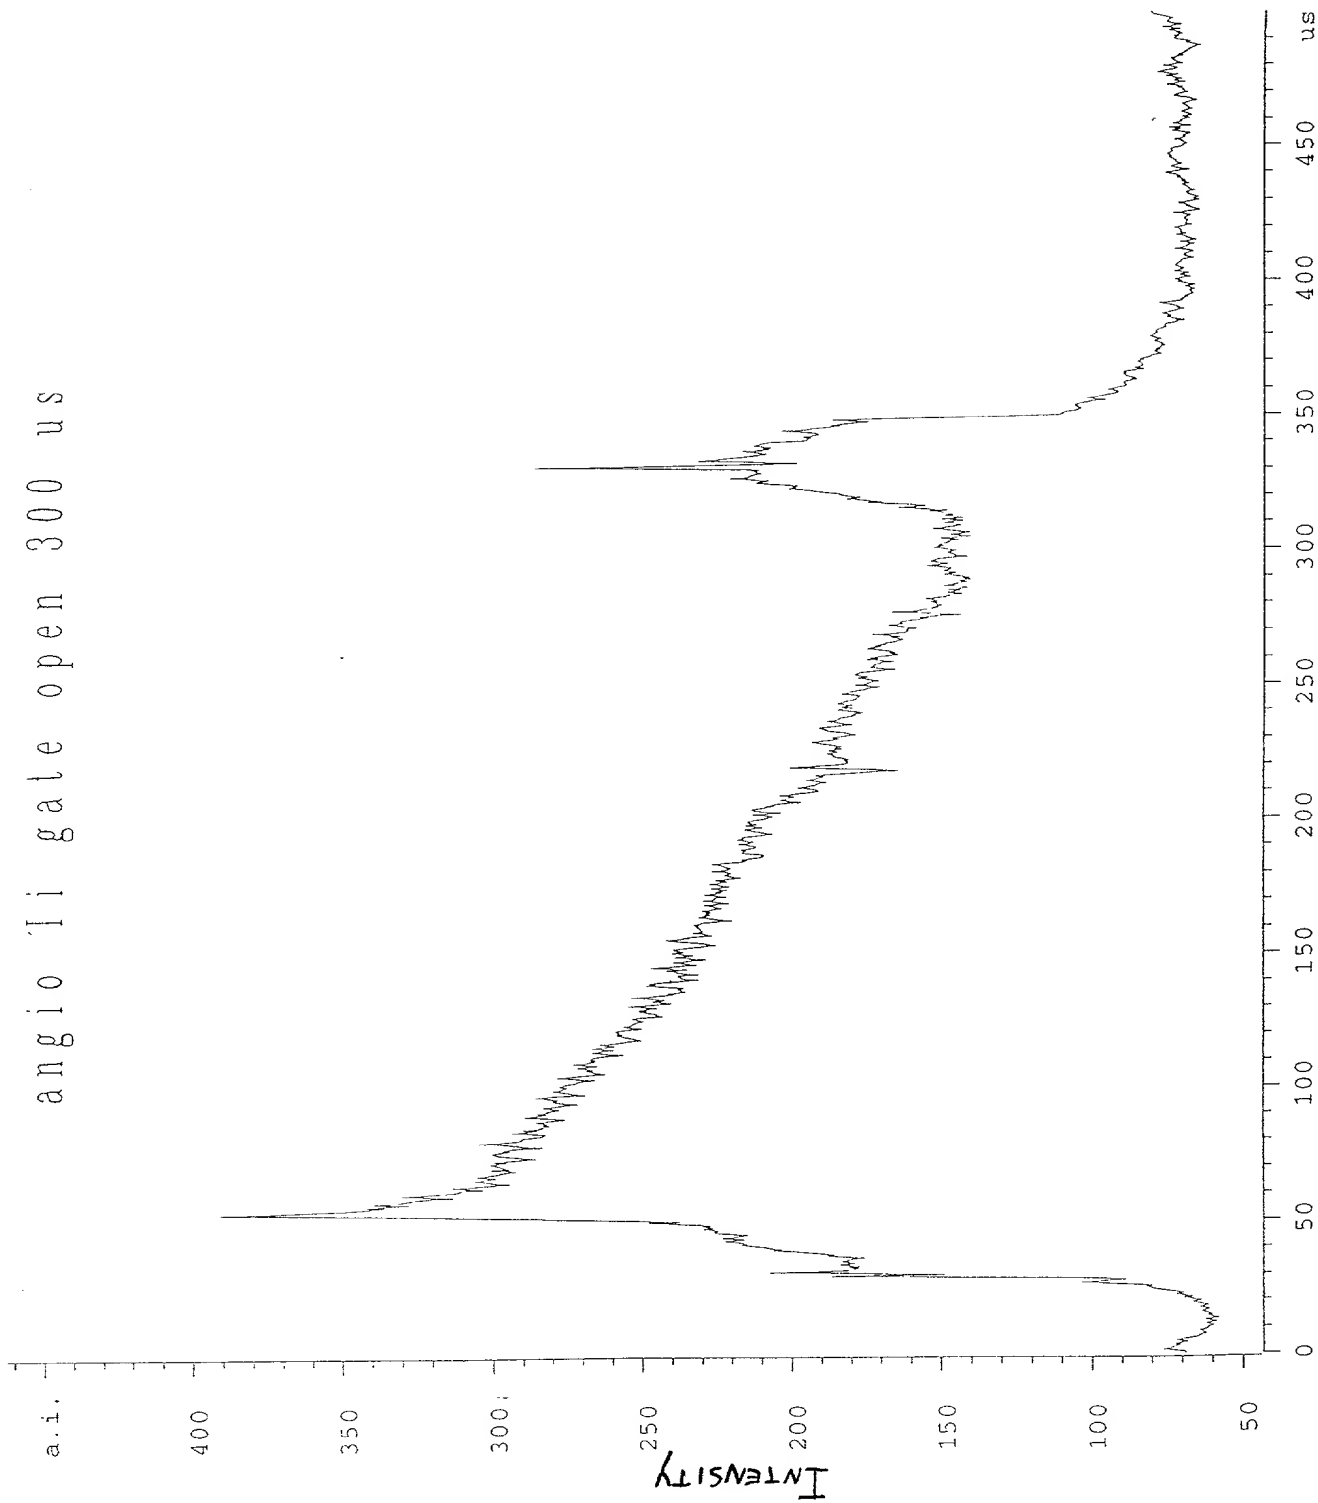


FIGURE 9

PULSE DURATION - MICROSECONDS